

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 16 2010

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130114

Name Kevin Stevenson ID# 2414 Date 03-12-10

A

Agency WAA Police Dept Phone # 907-786-1120

Instrument Location WAA Police Dept

B

Alco S/N 75470 Target Value .080 High Pressure 600

Alco Test Value Average .081 .080
1st Alco 2nd Alco

Signature [Signature]

(OVER)

BMB
3/24/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows. (Do Not write in the area below)



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 5th day of April, 2010.

[Signature]
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)

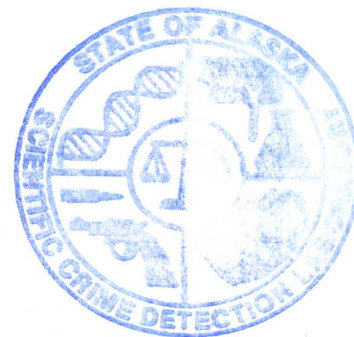

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N ~~130114~~ 130114

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130114
MARCH 12, 2010
OPERATOR'S NAME: STEVENSON KEVIN L.
OPERATOR'S NUMBER: 0414
SUBJECT'S LAST NAME:
VERIFICATION
SUBJECT'S FIRST NAME/MI:
VERIFICATION
O.L.N. #1 1234
DEPT/AGENCY: ANCD
CASE/REPORT: 03122010
TEST TYPE: U
ALCO TARGET VALUE: .080
ALCO S/N: 75470
--- BREATH ANALYSIS ---
.080 ADJUSTED FOR 29.54 in
ALCO TARGET .078 22:14
BLANK TEST .000 22:15
INTERNAL STANDARD VERIFIED 22:15
ALCO TO 29.54 in .081 22:16
BLANK TEST .000 22:16
SUBJECT SAMPLE .000 22:17
BLANK TEST .000 22:18
ALCO TO 29.54 in .080 22:18
BLANK TEST .000 22:19

8mb 3/24/10

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130114
MARCH 12, 2010
TIME 22:10
--- DIAGNOSTIC CHECK ---
COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 41c
BAROMETER: 29.54 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY
PRINTER TEST
"#####"
HIJKL NOPQRSTU VWXYZ 1234567890 abcdefghijklmno
pqrstuvwxy z0123456789